



ARTIFICIALIRIS CUSTOMFLEX® Extra life-changing results



Photodirectives for ordering
ARTIFICIALIRIS CUSTOMFLEX®



Content:

Why is the image/photo extract so important?

Which photo prints are needed?

How is a good picture taken?

How are photos evaluated?

Disclaimer

Summary


ARTIFICIALIRIS - EXtra life-changing results

Why is the image/photo extract so important?

Purpose:

Since the manufacutere is not able to see the patient's natural iris, it is necessary to rely on the pictures sent in with the order for a **ARTIFICIALIRIS CUSTOMFLEX®**.

The color of every computer screen and printer appears different as a result on a photo. Therefore, it is always necessary to **evaluate the printout** (hard copy).

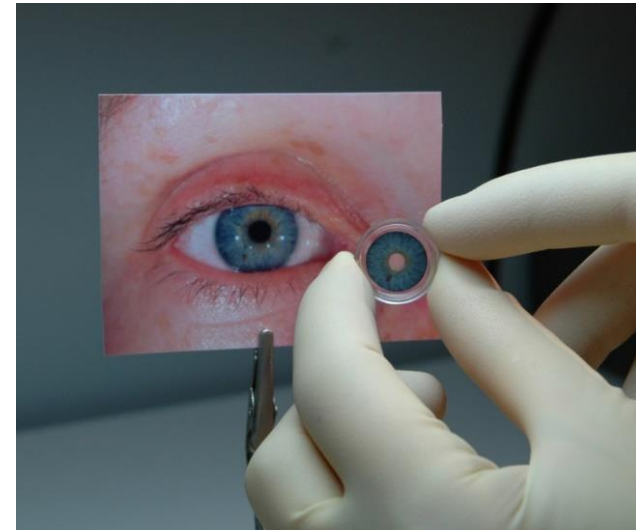

Important:

- The quality of the photo prints is crucial for a natural post-operative appearance of the patient's eye.
- HumanOptics reserves the right to refuse orders if the required patient images do not meet the necessary requirements.

ARTIFICIALIRIS - EXtra life-changing results

Which photo prints are needed?

Which photo prints are needed?




For production and clinical discussion, it is best to have an image of both eyes as a bridge photo and as a single photo.

ARTIFICIALIRIS - EXtra life-changing results

Which photo prints are needed?

Sizing of the iris on the picture

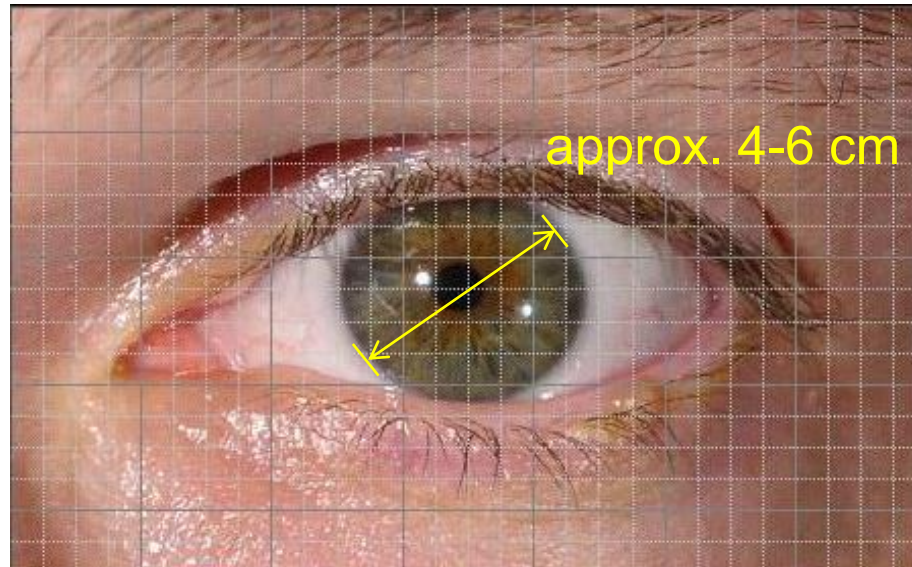

Standardized picture:

- Size of photo 9 x 13 cm (3.5 x 5“)
- Size of iris approx. 4 – 6 cm (1.5 – 2.5“)

ARTIFICIALIRIS - EXtra life-changing results

Which photo prints are needed?

Exception: No iris present on both sides (e.g. congenital aniridia)

As there are no iris remnants that can be reproduced in the production process, the patient can choose their own shade guide by ...

- using the **ARTIFICIALIRIS SELECT** color chart to select the desired shade
- selecting a close-up of an iris from a magazine
- using a close-up, e.g. of a relative's eyes, for the order



ARTIFICIAL*IRIS* - EXtra life-changing results

How is a good picture taken?

Procedure:

1. **Illuminate** the eye of the patient **evenly**, so that **no shadows** appear on the iris.
2. Carry out the **white balance** with the camera at the exact location where the photo of the patient's eye is to be taken. A gray or white card is required for this.
3. The patient's iris should be **completely** recognizable and **sharply** focused.

ARTIFICIALIRIS - EXtra life-changing results

How is a good picture taken?

Principles:

Good, even illumination of the eye is essential

Ideally use:

- Flash with softbox or ring flash → Note: regular flash can overexpose the photo and cause reflexes
- or:
- Continuous light at approx. 3200 Kelvin


When using a slit lamp, please ensure that the eye is not overexposed and that the images are very well resolved.

Important: Fundus cameras or other video cameras are **not** suitable for taking good photos. If you do not have the necessary equipment, you can also refer your patient to a **professional photographer**.

ARTIFICIAL IRIS - EXtra life-changing results

How is a good picture taken?

- Conjunctiva has a reddish color
- Iris color is greenish
- Picture seems underexposed

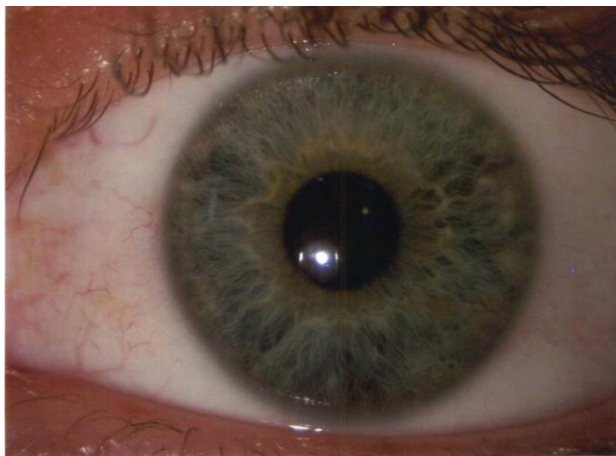

Both time the same patient,

Difference:

Illumination of the eye


- Conjunctiva is white with visible blood vessels
- Iris color appears in a clear blue shade



ARTIFICIAL IRIS - EXtra life-changing results

How is a good picture taken?

All colors are washed out,
details are not
recognizable

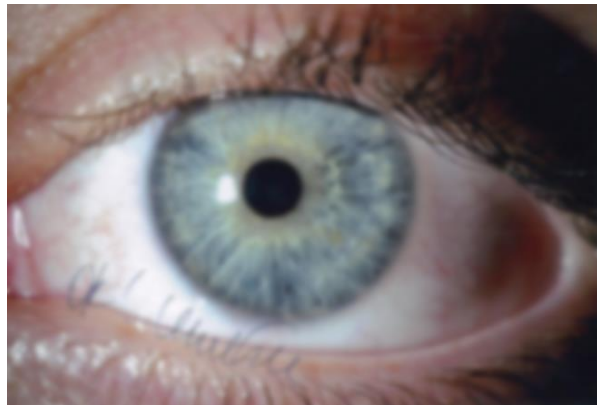


Both time the same
patient,

Difference:

Image sharpness

- All structures can be seen in detail
- The colors are recognizable in great detail and can be precisely identified



ARTIFICIAL *IRIS* - EXtra life-changing results

How is a good picture taken?

What are the most important aspects when taking and evaluating the image?

- ✓ **Illumination** of the eye
- ✓ **Size** of the iris on the image
- ✓ Image **sharpness**
- ✓ Only **photographic paper** may be used for the printout and this must be compared with the natural iris. If desired, **professional photographers** can help with the image creation
- ✓ Only **one** image is to be signed, which is to be used for the production



Example for a perfect picture for production

ARTIFICIALIRIS - EXtra life-changing results

How are photos evaluated?

Qualification of the production template

- Compare the photo with the natural iris under the same lighting conditions.
- Hold the photo printout directly next to the patient's eye.
- Compare whether the conjunctiva is white in the photo.
- Compare the patient's skin color in the photo with the natural skin color.
- Do the color patterns of the natural iris match those on the photo printout?



ARTIFICIALIRIS - EXtra life-changing results

How are photos evaluated?

Important note:

Orders can only be processed if the **required documents** are **complete!** The photo prints must be available as **hard copies** on **photographic paper** and comply with the photo guidelines. In addition, only one **image** of the healthy eye that is to be used for production may be **signed**.



CUSTOMFLEX® ARTIFICIALIRIS
ORDER FORM

FROM
Surgeon's name: _____
Clinic address: _____
Phone/Fac: _____
Email: _____

PLEASE SEND
To: _____
DISTRIBUTED BY: _____

I, the undersigned, hereby order a custom-made ARTIFICIALIRIS as follows:
Surgeon certifies me:
You will receive your personal certificate number after completion of the Order Certification Course.

Patient ID: _____

Eye to be treated: RE LE

Aniridia type: congenital acquired

Model selection:
 ARTIFICIALIRIS with Fiber
 ARTIFICIALIRIS Fiber Free

Standby selection:
 with one or with two standby implants

Please read the specific material to verify that we primarily offer supply if you will be charged for the 1st year of the treatment and a invoice will automatically be sent to you after 1 month.
Tough lens (10.0-12.5 mm or 12.5 mm depth) are available on request (certain conditions apply).
Please contact our customer service to check your supply options.

Please ensure that you enclosed the following documents to your order and make sure they comply with our photo directives:

Check list:
 Photo printout for production
 Photo printout of both eyes together (for reference)

Date: _____ Surgeon Signature (mandatory): _____ Patient Signature (optional): _____





ARTIFICIAL*IRIS* - EXtra life-changing results



Disclaimer

- The color of a **ARTIFICIAL*IRIS* CUSTOMFLEX®** corresponds to the photo template, but slight color deviations are possible due to the individual manual color application process.
- The appearance and color of the **ARTIFICIAL*IRIS*** in air is slightly darker compared to the product delivered in saline solution and in the eye after implantation.
- Ambient lighting can affect the appearance, color or luminosity of the product
- **ARTIFICIAL*IRIS* SELECT** Color Chart- The colors printed on the color chart were all photographed in saline solution. The colors of the prints in the color chart may differ slightly from the actual product due to the manual dyeing process during production.

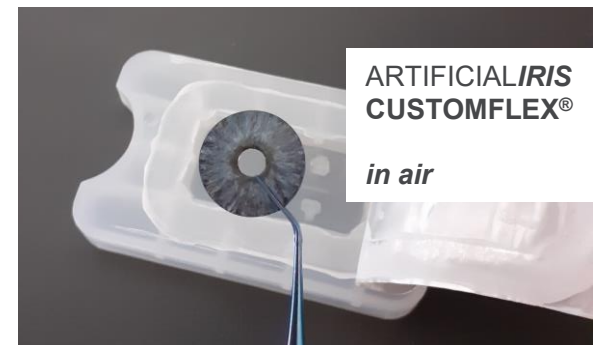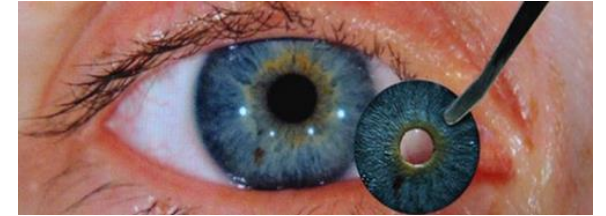

ARTIFICIALIRIS - EXtra life-changing results

Summary



- ✓ A **good photo** print is the key to a perfect color-matching ARTIFICIALIRIS CUSTOMFLEX®
- ✓ The **right equipment** is essential for taking good photos.
- ✓ **Only you** on site can check that the photo print matches the natural iris



Photodirectives
ARTIFICIAL *IRIS* CUSTOMFLEX®